

# Bi-Lateral Comparison between NIS-Egypt and NMISA-South Africa for the Calibration of an Optical Spectrum Analyzer

Osama Terra, Hatem Hussein, Adriaan Van Brakel

**Abstract**—Dense wavelength division multiplexing (DWDM) technology requires tight specification and therefore measurement of wavelength accuracy and stability of the telecommunication lasers. Thus, calibration of the used Optical Spectrum Analyzers (OSAs) that are used to measure wavelength is of a great importance. Proficiency testing must be performed on such measuring activity to insure the accuracy of the measurement results. In this paper, a new comparison scheme is introduced to test the performance of such calibrations. This comparison scheme is implemented between NIS-Egypt and NMISA-South Africa for the calibration of the wavelength scale of an OSA. Both institutes employ reference gas cell to calibrate OSA according to the standard IEC/ BS EN 62129 (2006). The result of this comparison is compiled in this paper.

**Keywords**—OSA calibration, HCN gas cell, DWDM technology, wavelength measurement.

## I. INTRODUCTION

FIBER optical communication is still rapidly developing with the constant introduction of newer technologies to increase the communications bandwidth. The most widely used new technology is the DWDM [1]. DWDM requires tight specification and therefore measurement of wavelength accuracy and stability of communication lasers. This specification is required because of precise channel allocation and detection requirements. Up to 80 different laser wavelengths (optical channels within wavelength range of 1520-1570 nm) can be used in DWDM. This increases the communication bandwidth from about 1 Gb/s to about 100 Gb/s, which allows high speed data transmission.

OSAs are widely used to measure the absolute wavelength and spectral purity of laser sources which are used in DWDM. Calibration of OSA is necessary to ensure accurate measurement of laser characteristics. Characterization of laser sources is not only important for DWDM systems, but also for other telecommunication applications. For example, laser spectral purity determines the chromatic dispersion in an optical communication system and hence the bandwidth. Therefore, it is important to calibrate OSAs to assure its accurate measurements. The standard IEC/BS EN 62129

(2006) describes different methods for the calibration of an OSA [2]. One of the methods that can be easily implemented for the calibration of OSA is the use of a reference gas cell. The most commonly used reference gas cells in the telecommunication wavelength region are Hydrogen cyanide (carbon isotope 13) ( $\text{H}^{13}\text{C}^{14}\text{N}$ ) in the wavelength range 1522-1577 nm, Hydrogen cyanide (carbon isotope 12) ( $\text{H}^{12}\text{C}^{14}\text{N}$ ) in the wavelength range 1514-1570 nm, carbon monoxide (carbon isotope 12) ( $^{12}\text{C}^{16}\text{O}$ ) in the wavelength range from 1560-1595 nm, and carbon monoxide (carbon isotope 13) ( $^{13}\text{C}^{16}\text{O}$ ) in the wavelength range from 1595-1630 nm.

In this paper, a comparison has been made between NIS-Egypt and NMISA-South Africa for the calibration of the OSA wavelength scale. The calibration has been performed using reference gas cell according to the standard IEC/ BS EN 62129 (2006).

## II. BACKGROUND ABOUT OSA

The main block of a grating-based OSA is a monochromator [3]. Fig. 1 shows a basic configuration of a monochromator. The monochromator has a planar diffraction grating and two concave mirrors. The incident light from the optical fiber is made parallel by a collimating mirror, and diffracted at the diffraction grating. Then, this light reflects on a focusing mirror and dispersively forms a spectrum on the slit plane. Only the light with the intended wavelength will be focused at the slit and can pass through it.

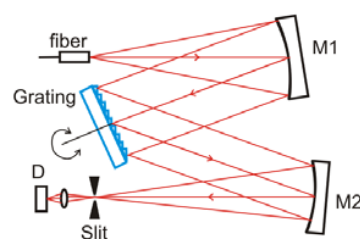


Fig. 1 Monochromator configuration, M1: collimating mirror, M2 focusing mirror, D: photodetector

The relation between the grating angle and wavelength has to be accurately determined and regularly calibrated for the accurate determination of the wavelength. Due to the nonlinearity of the grating rotation, this relation is not linear and therefore calibration over the whole intended wavelength range is required.

Osama Terra is with the National Institute of Standard (NIS), Tersa St. Haram, code:12211, P.O.Box: 136 Giza, Egypt (corresponding author, phone: +201141172900, e-mail: osama.terra@nis.sci.eg, osama.terra@gmail.com).

Hatem Hussein is with the NIS, Tersa St. Haram, code:12211, P.O.Box: 136 Giza, Egypt.

Adriaan Van Brakel is with the National Metrology Institute of South Africa (NMISA), Lynnwood Ridge, Pretoria, South Africa.

### III. REFERENCE GAS CELLS

Both NIS and NMISA employ reference gas cells to calibrate the wavelength scale of an OSA according to the standard IEC/BS EN 62129 (2006) [2]. However, NIS uses Hydrogen Cyanide ( $\text{H}^{13}\text{C}^{14}\text{N}$ ) gas cell that covers the wavelength range 1530-1557 nm, while NMISA uses a gas mixture from Hydrogen-Cyanide 12 ( $\text{H}^{12}\text{C}^{14}\text{N}$ ) and Carbon-Monoxide 12 ( $^{12}\text{C}^{16}\text{O}$ ) that covers the wavelength range 1515-1995 nm. The absorption lines with wavelengths from 1530-1560 nm are selected for the comparison. Table I shows the gas cells absorption lines that will be used for OSA calibration as reported by the manufacturer and measured by the others [4], [5].

TABLE I  
THE WAVELENGTHS OF THE GAS CELLS ABSORPTION LINES THAT WILL BE USED FOR OSA CALIBRATION

| $\text{H}^{13}\text{C}^{14}\text{N}$ |                          | $\text{H}^{12}\text{C}^{14}\text{N}$ |                          |
|--------------------------------------|--------------------------|--------------------------------------|--------------------------|
| R branch Wavelength (nm)             | P branch Wavelength (nm) | R branch Wavelength (nm)             | P branch Wavelength (nm) |
| 1533.14868                           | 1534.52984               | 1533.14868                           | 1534.52984               |
| 1532.47395                           | 1535.23629               | 1532.47395                           | 1535.23629               |
| 1531.80978                           | 1535.95333               | 1531.80978                           | 1535.95333               |
| 1531.15613                           | 1536.68095               | 1531.15613                           | 1536.68095               |
| 1530.51304                           | 1537.41922               | 1530.51304                           | 1537.41922               |
|                                      | 1538.16813               |                                      | 1538.16813               |
|                                      | 1538.92767               |                                      | 1538.92767               |
|                                      | 1539.69784               |                                      | 1539.69784               |
|                                      | 1540.47871               |                                      | 1540.47871               |
|                                      | 1541.27025               |                                      | 1541.27025               |
|                                      | 1542.07248               |                                      | 1542.07248               |
|                                      | 1542.88542               |                                      | 1542.88542               |
|                                      | 1543.70908               |                                      | 1543.70908               |
|                                      | 1544.54348               |                                      | 1544.54348               |
|                                      | 1545.38859               |                                      | 1545.38859               |
|                                      | 1546.24448               |                                      | 1546.24448               |
|                                      | 1547.11115               |                                      | 1547.11115               |
|                                      | 1547.9886                |                                      | 1547.9886                |
|                                      | 1548.87683               |                                      | 1548.87683               |
|                                      | 1549.7759                |                                      | 1549.7759                |
|                                      | 1550.68579               |                                      | 1550.68579               |
|                                      | 1551.60651               |                                      | 1551.60651               |
|                                      | 1552.53809               |                                      | 1552.53809               |
|                                      | 1553.48054               |                                      | 1553.48054               |
|                                      | 1554.43387               |                                      | 1554.43387               |
|                                      | 1555.3981                |                                      | 1555.3981                |
|                                      | 1556.37324               |                                      | 1556.37324               |
|                                      | 1557.3593                |                                      | 1557.3593                |
|                                      | 1558.35631               |                                      | 1558.35631               |
|                                      | 1559.36426               |                                      | 1559.36426               |

### IV. TRANSFER STANDARD

The transfer standard was an OSA purchased from Yokogawa with model AQ6370C. This OSA has a wavelength range of 600-1700 nm with resolution of 0.02 nm. Since OSA is heavy and contains optical component that cannot be easily transferred, the OSA is kept at NMISA while the reference absorption cell and the broadband source (the calibration

system) of NIS are transferred to NMISA. This means that, the same OSA will be calibrated using NIS and NMISA participants in the comparison at NMISA.

### V. OSA WAVELENGTH SCALE CALIBRATION

Reference gas cells are used to calibrate OSA. At NIS, the carbon 13 isotope of the Hydrogen Cyanide ( $\text{H}^{13}\text{C}^{14}\text{N}$ ) gas cell is used. The cell is purchased from *Traid technology* with specified gas pressure at 23 C of 100 Torr  $\pm$  5%, HCN purity of 98%, temperature dependence  $< 0.0001\text{nm}/^\circ\text{C}$  and wavelength accuracy of  $\pm 0.0003$  nm (1 sigma). In order to probe these absorption lines, an Erbium-doped fiber amplifier (EDFA) (QAMnet-gEDFA-17-2) is used as a broadband source. The EDFA emits a broad spectrum over the wavelength range (1530-1560 nm) with power  $> -30$  dBm/nm.



Fig. 2 OSA calibration setup using H13CN reference gas cell

At NMISA, the carbon 12 isotope of the Hydrogen Cyanide ( $\text{H}^{12}\text{C}^{14}\text{N}$ ) gas cell is used. A super luminescent diode (SLED) (EXFO (FSL2200SCL)) is used as a broadband source which has the wavelength range from 1460 nm to 1625 nm and power of more than  $-30$  dB.

### VI. RESULTS

Initially, NIS calibration system ( $\text{H}^{13}\text{C}^{14}\text{N} + \text{EDFA}$ ) is used to calibrate OSA. The calibration results are shown in Table II. Table II shows that the maximum error over the whole range is 8.4 pm with standard deviation of 1.7 pm. Thereafter, NMISA calibration system ( $\text{H}^{12}\text{C}^{14}\text{N} + \text{SLED}$ ) is used to calibrate OSA. The calibration results are shown in Table III. Table III shows that the maximum error over the whole range is 8.5 pm with standard deviation of 1.7 pm.

#### Uncertainty evaluation of distance scale calibration at NIS

The uncertainties of measurements were calculated according to the GUM [6] and guidelines as stipulated in the standard EN 62129 (2006) [2]. There are two main sources of uncertainty contributing to the uncertainty in the wavelength scale calibration of an OSA, namely, the uncertainty in the reference gas cell absorption lines and the standard deviation of the values measured during the calibration. According to the manufacturer and by [4], [5], which states the absorption lines of the HCN at zero pressure and the wavelength pressure dependence which is about 2 MHz/Torr and the measurement uncertainties therein, an upper limit for the uncertainty in the wavelength of the absorption lines is chosen to be  $\pm 3$  pm. The standard deviation from the calibration of the OSA according to section 6 is 1.7 pm for each cell. The combined uncertainty

is then equal to  $\pm 3.4$  pm. The expanded uncertainty at 95% is found to be  $\pm 6.8$  pm.

TABLE II  
OSA CALIBRATION WITH  $\text{H}^{13}\text{C}^{14}\text{N}$  GAS CELL

| R branch |           |           |                 | P branch |           |           |                 |
|----------|-----------|-----------|-----------------|----------|-----------|-----------|-----------------|
| Label    | OSA (nm)  | HCN (nm)  | $d\lambda$ (pm) | Label    | OSA (nm)  | HCN (nm)  | $d\lambda$ (pm) |
| R20      | 1530.2986 | 1530.3061 | 7.5             | P1       | 1543.1078 | 1543.1141 | 6.3             |
| R19      | 1530.7806 | 1530.7856 | 5               | P2       | 1543.8068 | 1543.8094 | 2.6             |
| R18      | 1531.27   | 1531.7738 | 4.9             | P3       | 1544.5126 | 1544.5147 | 2.1             |
| R17      | 1531.77   | 1531.7738 | 3.8             | P4       | 1545.226  | 1545.2300 | 4               |
| R16      | 1532.277  | 1532.2825 | 5.5             | P5       | 1545.9506 | 1545.9552 | 4.6             |
| R15      | 1532.793  | 1532.8010 | 8               | P6       | 1546.687  | 1546.6903 | 3.3             |
| R 14     | 1533.3234 | 1533.3292 | 5.8             | P7       | 1547.4344 | 1547.4353 | 0.9             |
| R13      | 1533.8612 | 1533.8671 | 5.9             | P8       | 1548.1862 | 1548.1904 | 4.2             |
| R12      | 1534.4102 | 1534.4149 | 4.7             | P9       | 1548.95   | 1548.9555 | 5.5             |
| R11      | 1534.9686 | 1534.9724 | 3.8             | P10      | 1549.7254 | 1549.7306 | 5.2             |
| R10      | 1535.5338 | 1535.5397 | 5.9             | P11      | 1550.5122 | 1550.5156 | 3.4             |
| R9       | 1536.1084 | 1536.1168 | 8.4             | P12      | 1551.305  | 1551.3106 | 5.6             |
| R8       | 1536.6968 | 1536.7037 | 6.9             | P13      | 1552.1088 | 1552.1156 | 6.8             |
| R7       | 1537.2956 | 1537.3004 | 4.8             | P14      | 1552.926  | 1552.9309 | 4.9             |
| R6       | 1537.9028 | 1537.9067 | 3.9             | P15      | 1553.7518 | 1553.7559 | 4.1             |
| R5       | 1538.5164 | 1538.5233 | 6.9             | P16      | 1554.5856 | 1554.5912 | 5.6             |
| R4       | 1539.141  | 1539.1494 | 8.4             | P17      | 1555.4306 | 1555.4365 | 5.9             |
| R3       | 1539.7774 | 1539.7856 | 8.2             | P18      | 1556.288  | 1556.2919 | 3.9             |
| R2       | 1540.426  | 1540.4314 | 5.4             | P19      | 1557.1538 | 1557.1573 | 3.5             |
| R1       | 1541.0824 | 1541.0873 | 4.9             | P20      | 1558.027  | 1558.0329 | 5.9             |
| R0       | 1541.7462 | 1541.7530 | 6.8             | P21      | 1558.913  | 1558.9185 | 5.5             |
|          |           |           |                 | P22      | 1559.8112 | 1559.8143 | 3.1             |

TABLE III  
OSA CALIBRATION WITH  $\text{H}^{12}\text{C}^{14}\text{N}$  GAS CELL

| R branch |           |           |                 | P branch |           |           |                 |
|----------|-----------|-----------|-----------------|----------|-----------|-----------|-----------------|
| Label    | OSA (nm)  | HCN (nm)  | $d\lambda$ (pm) | Label    | OSA (nm)  | HCN (nm)  | $d\lambda$ (pm) |
| R4       | 1530.5058 | 1530.5130 | 7.2             | P1       | 1534.5274 | 1534.5298 | 2.4             |
| R3       | 1531.1512 | 1531.1561 | 4.9             | P2       | 1535.2306 | 1535.2363 | 5.7             |
| R2       | 1531.805  | 1531.8098 | 4.8             | P3       | 1535.9476 | 1535.9533 | 5.7             |
| R1       | 1532.467  | 1532.4740 | 7               | P4       | 1536.675  | 1536.6809 | 5.9             |
| R0       | 1533.1402 | 1533.1487 | 8.5             | P5       | 1537.4162 | 1537.4192 | 3               |
|          |           |           |                 | P6       | 1538.1646 | 1538.1681 | 3.5             |
|          |           |           |                 | P7       | 1538.9238 | 1538.9277 | 3.9             |
|          |           |           |                 | P8       | 1539.6912 | 1539.6978 | 6.6             |
|          |           |           |                 | P9       | 1540.475  | 1540.4787 | 3.7             |
|          |           |           |                 | P10      | 1541.268  | 1541.2703 | 2.3             |
|          |           |           |                 | P11      | 1542.0682 | 1542.0725 | 4.3             |
|          |           |           |                 | P12      | 1542.8806 | 1542.8854 | 4.8             |
|          |           |           |                 | P13      | 1543.7066 | 1543.7091 | 2.5             |
|          |           |           |                 | P14      | 1544.5402 | 1544.5435 | 3.3             |
|          |           |           |                 | P15      | 1545.3838 | 1545.3886 | 4.8             |
|          |           |           |                 | P16      | 1546.2394 | 1546.2445 | 5.1             |
|          |           |           |                 | P17      | 1547.1082 | 1547.1112 | 3               |
|          |           |           |                 | P18      | 1547.9852 | 1547.9886 | 3.4             |
|          |           |           |                 | P19      | 1548.8716 | 1548.8768 | 5.2             |
|          |           |           |                 | P20      | 1549.7716 | 1549.7759 | 4.3             |
|          |           |           |                 | P21      | 1550.6848 | 1550.6858 | 1               |
|          |           |           |                 | P22      | 1551.6036 | 1551.6065 | 2.9             |
|          |           |           |                 | P23      | 1552.5334 | 1552.5381 | 4.7             |
|          |           |           |                 | P24      | 1553.4778 | 1553.4805 | 2.7             |

## VII. MEASUREMENTS COMPARED

The average of the wavelength deviation ( $d\lambda$ ) from Table II is compared to the average of that from Table III to evaluate the results of both institutes (NIS and NMISA). The comparison is given in Table IV.

| Parameter  |             | NIS          | NMISA        |
|------------|-------------|--------------|--------------|
| Wavelength | Value       | 8.4 pm       | 8.5 pm       |
|            | Uncertainty | $\pm 6.8$ pm | $\pm 6.8$ pm |

The wavelength calibration results are also plotted in Fig. 3.

Actually, the best way to compare the result is to use the normalized Error ( $E_n$ ). The normalized error is calculated according to:

$$E_n = \frac{\lambda_{NIS} - \lambda_{NMISA}}{\sqrt{(U_{NIS}^2 + U_{NMISA}^2)}} \quad (1)$$

where  $\lambda_{NIS}$ ,  $\lambda_{NMISA}$  are the wavelength measurement results by OSA at NIS and at NMISA,  $U_{NIS}$ ,  $U_{NMISA}$  are the expanded uncertainty of the wavelength measurement by OSA at NIS and NMISA. But, since the transitions wavelengths are not matched, the reference values of the wavelengths from the publications are used. Therefore, the equation becomes:

$$E_n = \frac{(\lambda_{NIS} - \lambda_{R,NIS}) - (\lambda_{NMISA} - \lambda_{R,NMISA})}{\sqrt{(U_{NIS}^2 + U_{NMISA}^2)}} \quad (2)$$

where  $\lambda_{R,NIS}$  is the reference value for the  $H^{13}C^{14}N$  cell, and  $\lambda_{R,NMISA}$  is the reference value for the  $H^{12}C^{14}N$  cell. If both values were equal, (2) will be (1). Some transitions are chosen from Tables II and III that are near to each other and distributed along the wavelength range.

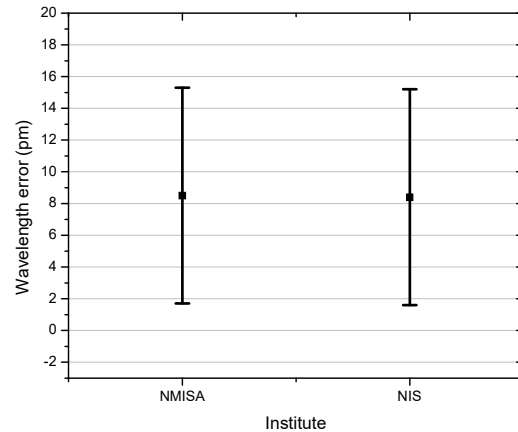


Fig. 3 Wavelength scale calibration comparison between NIS and NMISA for wavelength range 1530-1560 nm

TABLE V  
CALCULATION OF THE NORMALIZED ERROR  $E_n$

| NIS ( $H^{13}C^{14}N$ ) |           |                 | NMISA ( $H^{12}C^{14}N$ ) |           |                 | $E_n$ |
|-------------------------|-----------|-----------------|---------------------------|-----------|-----------------|-------|
| OSA (nm)                | HCN (nm)  | $d\lambda$ (pm) | OSA (nm)                  | HCN (nm)  | $d\lambda$ (pm) |       |
| 1530.2986               | 1530.3061 | 7.5             | 1530.5058                 | 1530.5130 | 7.2             | 0.03  |
| 1531.77                 | 1531.7738 | 3.8             | 1531.805                  | 1531.8098 | 4.8             | -0.10 |
| 1532.793                | 1532.8010 | 8               | 1532.467                  | 1532.4740 | 7               | 0.10  |
| 1534.4102               | 1534.4149 | 4.7             | 1534.5274                 | 1534.5298 | 2.4             | 0.24  |
| 1536.1084               | 1536.1168 | 8.4             | 1535.9476                 | 1535.9533 | 5.7             | 0.28  |
| 1536.6968               | 1536.7037 | 6.9             | 1536.675                  | 1536.6809 | 5.9             | 0.10  |
| 1537.2956               | 1537.3004 | 4.8             | 1537.4162                 | 1537.4192 | 3               | 0.19  |
| 1538.5164               | 1538.5233 | 6.9             | 1538.1646                 | 1538.1681 | 3.5             | 0.35  |
| 1539.7774               | 1539.7856 | 8.2             | 1539.6912                 | 1539.6978 | 6.6             | 0.17  |
| 1540.426                | 1540.4314 | 5.4             | 1540.475                  | 1540.4787 | 3.7             | 0.18  |
| 1543.8068               | 1543.8094 | 2.6             | 1543.7066                 | 1543.7091 | 2.5             | 0.01  |
| 1544.5126               | 1544.5147 | 2.1             | 1544.5402                 | 1544.5435 | 3.3             | -0.12 |
| 1545.226                | 1545.2300 | 4               | 1545.3838                 | 1545.3886 | 4.8             | -0.08 |
| 1548.1862               | 1548.1904 | 4.2             | 1547.9852                 | 1547.9886 | 3.4             | 0.08  |
| 1548.95                 | 1548.9555 | 5.5             | 1548.8716                 | 1548.8768 | 5.2             | 0.03  |
| 1549.7254               | 1549.7306 | 5.2             | 1549.7716                 | 1549.7759 | 4.3             | 0.09  |
| 1550.5122               | 1550.5156 | 3.4             | 1550.6848                 | 1550.6858 | 1               | 0.25  |
| 1551.305                | 1551.3106 | 5.6             | 1551.6036                 | 1551.6065 | 2.9             | 0.28  |
| 1552.926                | 1552.9309 | 4.9             | 1552.5334                 | 1552.5381 | 4.7             | 0.02  |
| 1553.7518               | 1553.7559 | 4.1             | 1553.4778                 | 1553.4805 | 2.7             | 0.15  |

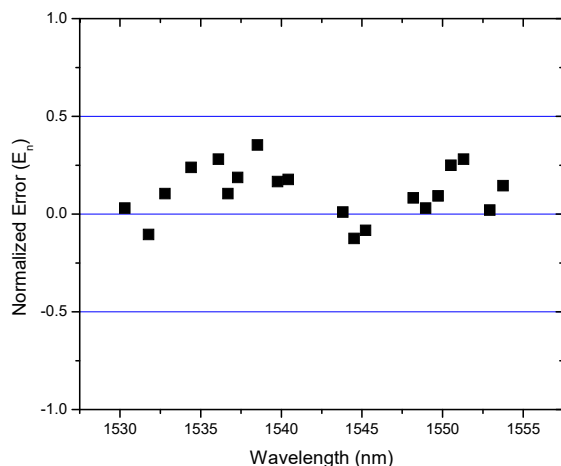


Fig. 4 Normalized Error  $E_n$  for comparison of both institute results

### VIII. CONCLUSION

A bi-lateral comparison between NIS-Egypt and NMISA-South Africa in the calibration of the wavelength scale of OSA has been conducted. A transfer OSA has been calibrated by both institutes, NIS and NMISA for the wavelength scales using their respective standards according to the IEC/EN standard 62129 (2006). Good agreement is found between the results from both institutes which lie within the uncertainty limits of the OSA.

### ACKNOWLEDGMENT

The author would like to thank the Science and Technology Development Fund (STDF) for supporting and funding this research and the accreditation process under the umbrella of center of excellence projects-laboratory accreditation.

### REFERENCES

- [1] R. Antil, Pinki, S. Beniwal, "An Overview of DWDM Technology & Network", International Journal of Scientific & Technology Research, volume 1, issue 11, December (2012).
- [2] IEC/EN/BS standard, "Calibration of optical spectrum analyzers", IEC/BS EN 62129 (2006).
- [3] M. Kojima, T. Mori, T. Kaneko, T. Yamamoto, A. Horiguchi, G. Ishihara, "High-speed Measurement Technologies of AQ6370C Optical Spectrum Analyzer", Yokogawa Technical Report, Vol.55 No.1 (2012).
- [4] W. C. Swann and S. L. Gilbert, "Line centres, pressure shift, and pressure broadening of 1530–1560 nm hydrogen cyanide wavelength calibration lines", J. Opt. Soc. Am. B., Vol. 22, No. 8, August (2005).
- [5] H. Sasada and K. Yamada, "Calibration lines of HCN in the 1.5-Mum region", Applied optics, Vol. 29, No. 24 (1990).
- [6] BIPM/IEC/ISO. "Guide to the Expression of Uncertainty in Measurement". ISBN9267101889 (1995).