

# Highly Sensitive Label Free Biosensor for Tumor Necrosis Factor

Tze Sian Pui, Tushar Bansal, Patthara Kongsuphol, Sunil K. Arya

**Abstract**—We present a label-free biosensor based on electrochemical impedance spectroscopy for the detection of pro-inflammatory cytokine Tumor Necrosis Factor (TNF- $\alpha$ ). Secretion of TNF- $\alpha$  has been correlated to the onset of various diseases including rheumatoid arthritis, Crohn's disease etc. Gold electrodes were patterned on a silicon substrate and self assembled monolayer of dithiobis-succinimidyl propionate was used to develop the biosensor which achieved a detection limit of  $\sim 57$ fM. A linear relationship was also observed between increasing TNF- $\alpha$  concentrations and charge-transfer resistance within a dynamic range of 1pg/ml – 1ng/ml.

**Keywords**—Tumor necrosis factor, electrochemical impedance spectroscopy, label free, self assembled monolayer

## I. INTRODUCTION

PATHOGEN specific T-cells are a hallmark of specific immunity and are crucial for the protective effect of a vaccine. When a vaccinated individual encounters a pathogen, these “educated” or “memory” T-cells respond rapidly by secreting cytokines that orchestrate an immune system fightback. Cytokines are a family of regulatory proteins which are mostly produced by activated macrophages and trigger immune-mediated inflammatory responses within the body via intercellular signaling. In healthy individuals, cytokines tend to be low (usually in pg/ml concentrations). However, at the onset of a pathological condition such as dengue, arthritis etc. these levels get elevated ten to hundredfold, triggering local cell apoptosis.

Efforts are being made to utilize cytokines as therapeutic and vaccine targets [1]. However, more research is needed to accurately assign specific profiles to specific diseases and to use cytokine-secreting cells as prognostic markers. So far, studies have mostly been performed at a small scale because of complicated sample preparation and manual operation steps [2]. Additionally, the time required to perform flow cytometry [3] makes it impossible to analyze hundreds and thousands of samples. Yet, information about the nature of cytokine-secreting cells could be of immense diagnostic value.

Measurement of serum cytokines can also provide information about the magnitude of the overall immune activation in a patient. Recently, it was demonstrated that there is indeed a correlation between serum and cell-secreted cytokines [4]. Bead-arrays are primarily used to measure the concentrations of cytokines in the serum [5]. However, serum cytokines do not provide any information about specific protection if the source of the cells is unknown.

Whereas the protective or pathological function of these cell subsets have mostly been studied in mice, a comprehensive T-cell analysis has become a standard readout to test the efficacy of vaccines, including dengue vaccine candidates [6,7].

Conventionally, cytokines are measured using ELISA. Such fluorescent labeling systems are highly-sensitive but are often expensive and time consuming contributing to the difficulty of diagnosing the disease quickly.

Immunological research has seen an enormous progress in the identification and functional characterization of immune cell subsets and T-cells in particular, using mostly multiparametric flow cytometry as the method of choice. Currently, the only routine analytical assay based on cell type-specific cytokines is the Quantiferon test, which is used to diagnose TB infection by detecting TB-specific T-cells [8].

Only selected clinical laboratories are able to perform this time-consuming and labor-intensive test. In clinical practice, one of the persistent problems with inflammatory therapy has been a lack of simple measuring tools which give an accurate picture of inflammatory stress.

Label-free immunosensors, in which interactions between antibody and antigen are directly monitored without the presence of fluorescent labels offer increased advantages of low cost, speed and simplicity over conventional methods. Electrochemical impedance spectroscopy (EIS) is a label free Faradaic impedance technique that is performed in the presence of a redox probe. Various other biomolecules such as proteins, nucleic acids etc. have been detected with EIS [9-13].

Excellent reviews on EIS technique and its applications are available elsewhere [14, 15]. EIS techniques combined with self assembled monolayer (SAM) have gained increased attention [16, 17, 18] as SAM allows a closer binding of biomolecules enabling EIS to detect the smallest of capacitance or resistance changes [19], resulting in improved detection. The advantages of EIS-based sensors over labeled approaches lie in their simple labeling protocol, high sensitivity and potential of mass fabrication for low cost diagnostic and therapeutic purposes in remote settings.

T-S. Pui is with the Institute of Microelectronics, A\*STAR, Singapore. (phone: 065-67705786; fax: 065-67731914; e-mail: puits@ime.a-star.edu.sg).

T. Bansal is with the Institute of Microelectronics, A\*STAR, Singapore. (phone: 065-67705727; fax: 065-67731914; e-mail: bansalt@ime.a-star.edu.sg).

P. Kongsuphol is with the Institute of Microelectronics, A\*STAR, Singapore. (phone: 065-67705607; fax: 065-67731914; e-mail: kongsuphol@ime.a-star.edu.sg).

S. K. Arya is with the Institute of Microelectronics, A\*STAR, Singapore. (phone: 065-67705621; fax: 065-67731914; e-mail: aryask@ime.a-star.edu.sg).

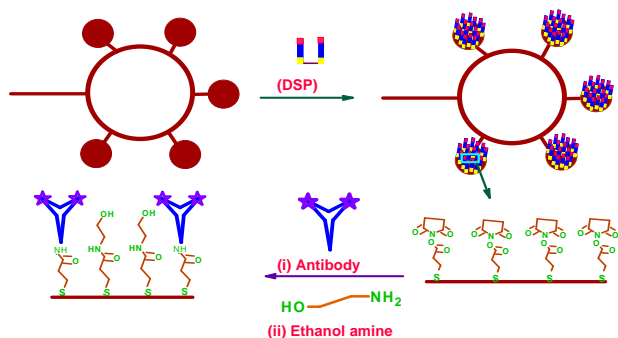


Fig. 1 Detailed steps of EA/anti-TNF- $\alpha$ /DSP/Au electrode functionalization process. Ethanol amine was used to prevent non-specific adsorption

Here we present a cheap and highly sensitive label-free immunosensor to detect TNF- $\alpha$ . Array of gold electrodes were fabricated on a silicon substrate with common photolithography processes. A self assembled monolayer of DSP was utilized to immobilize TNF- $\alpha$  antibodies and ethanol amine was used to prevent non-specific binding. Nyquist plots of EIS spectra indicated a proportional increase in charge-transfer resistance with increasing TNF- $\alpha$  concentration in the physiological range of 1pg/ml – 1ng/ml. A detection limit of ~57fM was achieved with minimal non-specific binding.

## II. PROCEDURE

### A. Materials and Chemicals

Tris(2-carboxyethyl) phosphine hydrochloride (TCEP), ethanol amine (EA) and dimethyl sulfoxide (DMSO) were obtained from Sigma Aldrich-USA. Human anti-TNF- $\alpha$ , target protein TNF- $\alpha$  and ELISA kit were purchased from Biolegend. Phosphate-buffered saline (PBS) and dithiobis-succinimidyl propionate (DSP) were purchased from Invitrogen and Proteochem respectively.

### B. Electrode fabrication

An array of circular gold microelectrodes with sensing areas having a diameter of 110  $\mu\text{m}$  each were fabricated on an 8" silicon wafer using standard photolithography techniques. Ti/Au (0.1 $\mu\text{m}$ /1.0 $\mu\text{m}$ ) layer was deposited using an electron-beam evaporator (Temescal Inc.). The sensing microelectrodes, bond pads, and connecting route lines were patterned by a series of processes such as photoresist spin coating (PFI-A26, Sumitomo Chemical Co., Ltd.), photolithography through a chrome mask in EVG 5200 Mask Aligner (EVG Group) and development in Shipley MF-319 developer (MicroChem Corp.). The unpatterned metal regions were etched with Au etchant (Au-600, CLC) and Ti etchant (Ti-890, CLC). Photoresist was then stripped in solvent and the wafers were cleaned in H<sub>2</sub>SO<sub>4</sub>:H<sub>2</sub>O<sub>2</sub> solution (4:1) at 125°C to remove residual contamination. Subsequently, the wafer was passivated with a moisture barrier layer SiO<sub>2</sub>/SiN (0.8 $\mu\text{m}$ /0.2 $\mu\text{m}$ ) through plasma enhanced chemical vapor deposition (PECVD).

### C. Immobilization of antibodies

Electrodes were pre-cleaned with acetone, ethanol, and copious amounts of de-ionized (DI) water. Afterwards, they were cleaned with piranha solution (H<sub>2</sub>SO<sub>4</sub>:H<sub>2</sub>O<sub>2</sub>; 7:3) for 5mins followed by rinsing in DI. For DSP SAM formation, 2 mg/ml solution of DSP in DMSO was prepared and reduced with 5mM TCEP for 15mins at 37°C. Chips were then incubated in DSP solution for 1hr at room temperature. After SAM formation, electrodes were rinsed with DMSO to remove any unbound DSP followed by rinsing in DI. The DSP modified electrodes were utilized immediately for immobilization of TNF- $\alpha$  antibodies (anti-TNF- $\alpha$ ) after their preparation. The antibodies were covalently attached to DSP SAM by incubating the active area of electrodes in 50 $\mu\text{l}$  of 50 $\mu\text{g}/\text{ml}$  antibodies in phosphate buffer saline (PBS) solution (1x, pH 7.4) for 1hr at room temperature. Covalent binding occurs via reaction between the amino group on the antibody and reactive succinimidyl group on DSP. The electrode (anti-TNF- $\alpha$ /DSP/Au) thus formed was washed thoroughly with 1% EA in PBS to block remaining DSP groups and to prevent any non-specific adsorption (Fig. 1). Prepared electrodes were stored at 4°C when not in use and were characterized using electrochemical impedance spectroscopy during experimentation.

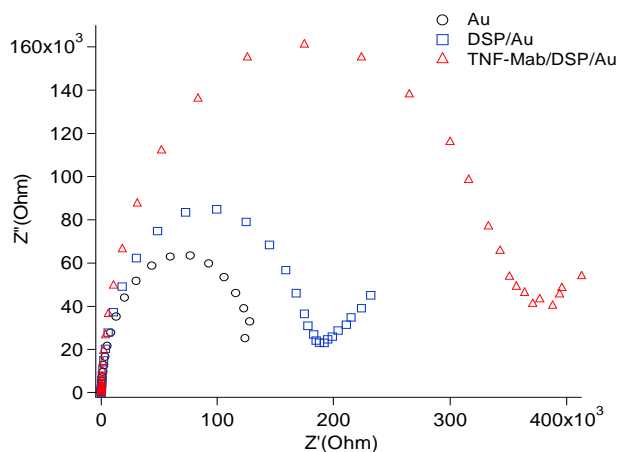


Fig. 2 Nyquist plots of (i) blank gold electrode (Au) (ii) DSP/Au electrode (iii) TNF- $\alpha$  monoclonal antibody/DSP/Au electrode. Diameter of the semicircle represents the charge-transfer resistance ( $R_{ct}$ ) on the electrode surface. Increase of  $R_{ct}$  with each process i) 140 k $\Omega$ , ii) 185 k $\Omega$  and iii) 370 k $\Omega$  indicates the retardation of the charge transfer process and therefore the successful modification of the surface

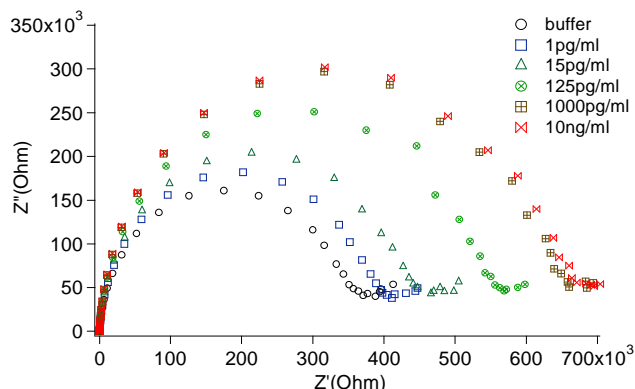


Fig. 3 Nyquist plots of EIS spectra on EA/anti-TNF- $\alpha$ /DSP/Au electrodes for buffer and 4 different concentrations of TNF- $\alpha$  in the range of 1pg/ml – 10ng/ml. A saturation effect was seen at 10ng/ml

#### D. EIS measurements

Autolab PGSTAT302 was used to record the changes in impedance. Concentrations of TNF- $\alpha$  from 1 pg/ml to 10ng/ml were prepared in 1x PBS containing 5mM ferrocyanide and 5mM of ferricyanide i.e. 5mM  $Fe(CN)_6^{3-/4-}$  as a redox probe. Electrodes were stored in PBS before use in EIS analysis. For AC sweep impedance measurements, initial potential of 0V, amplitude of 25mV and a frequency range of 1Hz – 1MHz was used.

### III. RESULTS AND DISCUSSION

Nyquist plots of impedance spectra on the gold electrodes after each modification (bare electrodes, after SAM functionalization and after antibody immobilization) were recorded and used for the characterization of electrode fabrication (Fig. 2). Diameter of the semicircle represents the charge-transfer resistance ( $R_{ct}$ ) on the electrode surface. Increase of  $R_{ct}$  with each process indicates the retardation of electron transfer and therefore the successful modification of the surface. Immobilization of monoclonal antibodies on gold electrodes had the biggest increase in electron charge transfer.

Fig. 3 shows the Nyquist plots of EIS spectra obtained on the EA/TNF- $\alpha$ /DSP/Au electrodes for 5 different TNF- $\alpha$  concentrations (1pg/ml – 10ng/ml) indicating a detection limit of  $\sim 57$ fM. A saturation effect was seen at levels above 1ng/ml that can be attributed to the saturating density of antibody on the electrodes and the wide range under consideration. Several detection methods including SAM based impedimetric immunosensors [20, 21], fluorescent microwells [22] and photonics [23] have been used for the detection of various cytokines including TNF- $\alpha$ . Cesaro-Tadic et al. [24] developed a miniaturized immunoassay using an independent capillary system. Although highly sensitive, their design employed immunofluorescence which is a costly approach.

Ganesh et al. [23] used a photonic crystal to develop a fluorescence sandwich immunoassay but the sensitivity of their system was very low (1ng/ml). All of these are costly methods requiring specialized equipment and multiple processing steps, and are not appropriate as low cost biosensors.

With increasing TNF- $\alpha$  concentration, diameter of the Nyquist plots was observed to increase as well, indicating that TNF- $\alpha$  binds to immobilized anti-TNF- $\alpha$  on the electrodes, producing a surface layer that decreases  $R_{ct}$  from solution to electrode surface in the presence of redox probe. A linear relationship was observed (Fig. 4) between changes in  $R_{ct}$  values and the log of TNF- $\alpha$  concentrations. Biosensor sensitivity can be increased at the expense of increasing electrode sizes and sensor area. However, we benchmarked our results against ELISA (Fig. 5) which yielded a detection limit of 15.6 pg/ml ( $\sim 890$  fM) indicating that our proposed biosensor design is already more sensitive than the conventional technique and works well within the physiological range.

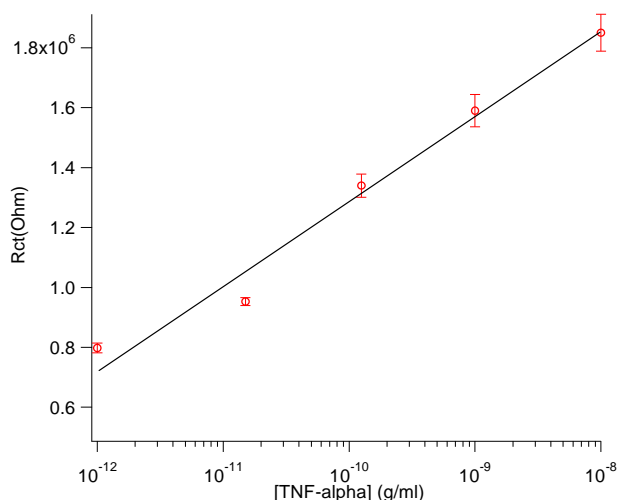


Fig. 4 Linear curve of charge-transfer resistance ( $R_{ct}$ ) obtained from EIS studies for 5 different TNF- $\alpha$  concentrations over 3 chips

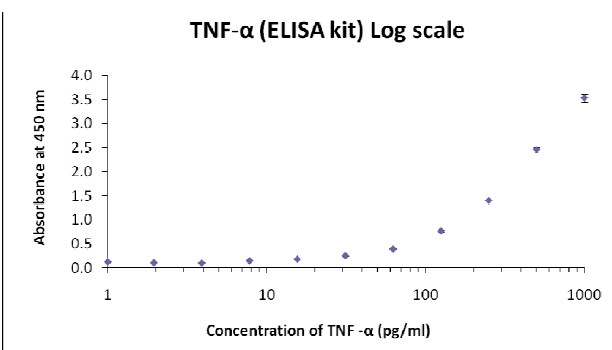


Fig. 5 Detection of TNF- $\alpha$  using ELISA kit. TNF- $\alpha$  was prepared at different concentrations (1 pg/ml – 1000 pg/ml) and was detected by ELISA. Optical density (OD) was read at 450 nm. Change in OD could be observed at 15.6 pg/ml and was undetectable at lower concentrations

To further understand and characterize complex cytokine networks and to make use of them as diagnostic and prognostic markers, a sensor system with the capabilities of simple operation, fast and quantitative detection of cell-specific cytokines secretion as well as with an affordable cost that can be used in large cohorts is indispensable.

## IV. CONCLUSION

In this work, we fabricated a low cost, easy to fabricate and sensitive biosensor to detect TNF- $\alpha$ . TNF- $\alpha$  is a cytokine that plays an important role in cell signaling during inflammation. Self assembled monolayer of dithiobis-succinimidyl propionate (DSP) was functionalized on gold electrodes and non-specific binding was prevented with ethanol amine (EA). The biosensor showed excellent selectivity and detection limit ( $\sim 57$ fM) compared to other cytokine sensor techniques. A linear relationship was found between the charge-transfer resistance and logarithmic value of the TNF- $\alpha$  concentrations in the physiological range (1pg/ml – 10ng/ml). We believe this biosensor may serve as a useful diagnostic and therapy monitoring tool for accurate monitoring of TNF- $\alpha$

## ACKNOWLEDGMENT

The authors would like to thank Wong Chee Chung for his input on fabrication methods and A\*STAR (Agency for Science Technology and Research), Singapore for providing support for this project (JCO grant# 11/03/FG/07/03).

## REFERENCES

- [1] J. Mongkolsapaya et al, *Nat Med*, 9, 921-927, 2003
- [2] World Health Organization, *Dengue: guidelines for diagnosis, treatment, prevention and control*, 2009
- [3] L. Diane et al, *Expert Review of Vaccines*, 8, 779-789, 2009
- [4] J. Jason et al, *Clin Diagn Lab Immunol.*, 8, 1097-1103, 2001
- [5] S. S. Khan, M. S. Smith, D. Reda, A. F. Suffredini, J. P. McCoy, *61B*, 35-39, 2004
- [6] F. Guirakhoo et al, *Hum Vaccin.*, 2, 60-67, 2006
- [7] B. Guy B, *Vaccine*, 26, 5712-5721, 2008
- [8] T. G. Connell, *PLoS ONE*, 3, e2624, 2008
- [9] R. Pei, Z. Cheng, E. Wang and X. Yang, *Biosensors and Bioelectronics*, 16, 355-361, 2001
- [10] J. Wang, E. Palecek, P. E. Nielsen, G. Rivas, X. Cai, H. Shiraishi, N. Dontha, D. Luo and P. A. M. Farias, *J. Am. Chem. Soc.*, 118, 7667-7670, 1996
- [11] W. C. I. Homs *Anal. Letters*, 35, 1875-1894, 2002
- [12] A. M. Oliveira-Brett, C. M. A. Brett and L. A. Silva, *Bioelectrochemistry*, 56, 33-35, 2002
- [13] C. M. A. Brett, A. M. O. Brett and S. H. P. Serrano, *Electrochimica Acta*, 44, 4233-4239, 1999
- [14] E. Katz and I. Willner, *Electroanalysis*, 15, 913-947, 2003
- [15] S-M. Park, J-S Yoo, *Anal Chem.*, 75, 455A-461A, 2003
- [16] E. Valera, J. R. Azcon, A. Rodríguez, L. M. Castaner, F. J. Sanchez and M. P. Marco, *Sensors and Actuators B*, 125, 526-537, 2007
- [17] J. R. Azcon, E. Valera, A. Rodríguez, A. Barranco, B. Alfaro, F. S. Baeza and M. P. Marco *Biosensors and Bioelectronics*, 23, 1367-1373, 2008
- [18] S. K. Arya, G. Chormokur, M. Venugopal and S. Bhansali, *Analyst*, 135, 1941-1946, 2010
- [19] S. K. Arya, G. Chormokur, M. Venugopal and S. Bhansali, *Biosensors and Bioelectronics*, 25, 2296-2301, 2010
- [20] M. Dijkstra, B. Kamp, J. C. Hoogvliet and W. P. Van Bennekom, *Anal. Chem.*, 73, 901-907, 2001
- [21] J. T. La Belle et al., *Biosensors and Bioelectronics*, 23, 428-431, 2007.
- [22] H. Zhu, G. Stybayeva, M. Macal, E. Ramanculov, M. D. George, S. Dandekar and A. Revzin, *Lab on chip*, 8, 2197-2205, 2008
- [23] N. Ganesh, I. D. Block, P. C. Mathias, W. Zhang, E. Chow, V. Malyarchuk and B. T. Cunningham, *Optics Express*, 16, 21626-21640, 2008
- [24] S. Cesaro-Tadic et al, *Lab on chip*, 4, 563-569, 2004

**Tze S. Pui** received his M.Sc. in Medical Physics in 2004 from the University of Malaya, Malaysia and Ph.D. degree in Biomedical Engineering in 2011 from the Nanyang Technological University, Singapore. He is currently a scientist at Institute of Microelectronics, A\*STAR, Singapore. His research interests include high throughput, high content screening systems for biological analysis, and electrical/electrochemical assays for cell based biosensing.

**Tushar Bansal** received his M.Sc. and Ph. D in Electrical Engineering in 2006 and 2009 resp. from the University of Michigan, Ann Arbor. He is currently a scientist at the Institute of Microelectronics, A\*STAR, Singapore. His research interests include high throughput drug screening systems, integrated lab-on-chip systems and developing label-free electrochemical biosensors.

**Patthara Kongsuphol** received her M.Sc. in Physiology from Mahidol University, Bangkok, Thailand in 2006 and received Ph.D. in Physiology from Regensburg University, Regensburg, Germany in 2011. She is currently a scientist at Institute of Microelectronics, A\*STAR, Singapore. Her research interest is in study of ion channel regulation and high through put screening techniques.

**Sunil K. Arya** received his M.Sc. in Organic Chemistry in 2004 and Ph.D. in Chemistry-Biosensor in 2008 from the University of Delhi, India. He is currently a scientist at the Institute of Microelectronics, A\*STAR, Singapore. He completed a post-doctorate at University of South Florida, Tampa, Florida, USA and at National Institute of Nanotechnology at University of Alberta, Edmonton, Alberta, Canada. His primary interests are in synthesis and applications of nanomaterials, monolayers and MEMS for gas sensor and electrochemical biosensor. His research focus is in the areas of micro/nanofabrication, materials science and thin film sensors/biosensor.